



# AURA SYSTEMS

HIGH-THROUGHPUT, FLUIDICS-FREE  
AGGREGATE AND PARTICLE  
CHARACTERIZATION AND IDENTIFICATION

- Particle ID
- Subvisible Aggregate Analysis
- DNA Leakage
- Polysorbate Degradation
- Product Purity
- 5  $\mu$ L – 10 mL Sample Volume

## An Aura For You




- Automation Ready
- Know Your Aggregates
- Sample Volumes That Meet Your Needs
- Fast Answers

- Fluidics-Free Peace of Mind
- Trustworthy Data with Minimal Optimization
- Easy Method Transfer
- Machine-Learning Free Aggregate ID

## Take the Guesswork Out of Your Aggregate ID


Don't waste time troubleshooting incorrectly identified aggregates in your therapeutic. Aura uses a combination of brightfield and fluorescent imaging to specifically ID and quantitate cell, viral capsid, protein, degraded excipients, and packaging contaminants so you'll know exactly what's in your sample.

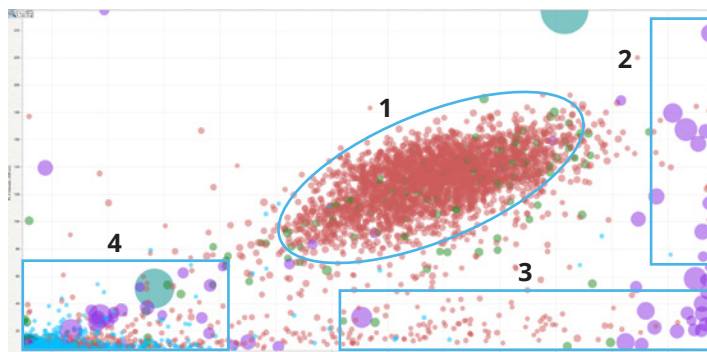

Identify cell doublets and triplets (1), cellular aggregates (2), protein aggregates (3), and plastic contaminants (4) in a cell therapeutic sample.

## Make the Best Decisions About Your Therapeutic

Know whether formulation or process modifications are needed to avoid aggregates that can affect the efficacy or safety of your drug therapeutics. [Fluorescence Membrane Microscopy \(FMM\)](#) uses specific fluorescent dyes or conjugated antibodies to help you visualize, quantitate, and ID aggregates, subvisible particles (SVP), and visible particles. Know for sure what is protein, viral capsid, cell, degraded polysorbate, plastic, or a fiber in your sample.

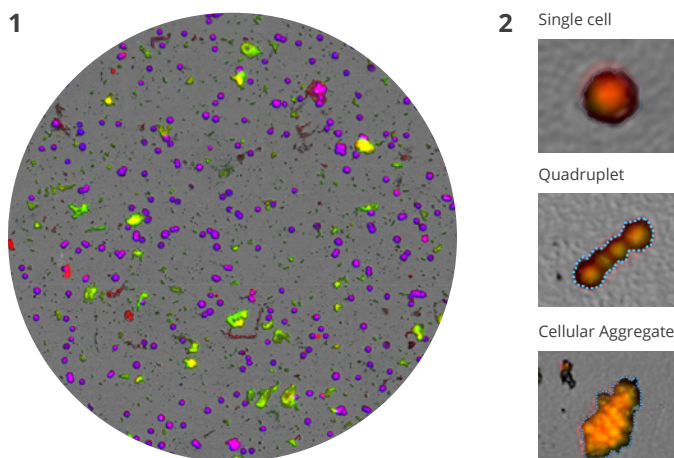


**1:** Distinguish cells (pink), protein aggregate (red), and particles labeled with a particle-specific conjugated antibody (yellow).

**2:** Cell aggregates can easily be mis-identified, but FMM can ID them with ease.

## Evaluate AAV and Payload Related Stability of Your Gene Therapy

Quantitate the stability of different AAV serotypes under several conditions. Or label free DNA with SYBR™ Gold to monitor increased subvisible particle formation that can occur when nucleic acids leak out of an unstable capsid. Assess the stability of your gene therapy throughout the entire development process – with just 5  $\mu$ L of sample!

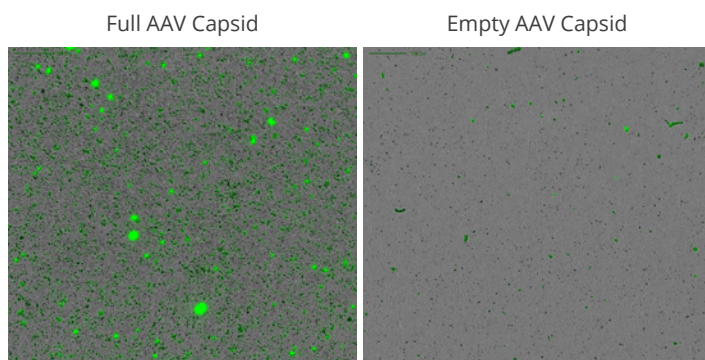

Label DNA with SYBR Gold (green) to monitor DNA leakage using FMM on Aura.


## Out of the Box ID

Using morphology to classify particles is notoriously unreliable and not everybody has the time or resources to build complicated machine learning libraries. Plus, these approaches just don't measure up when you have complex aggregates in your sample that are a combination of cell, protein, or plastic.

FMM makes it simple and straightforward to specifically ID cell from non-cell and protein from non-protein. Now, you can finally know what's in your sample without having to spend hours sorting through images. The specificity of FMM makes it easy to distinguish what's what in complex samples, so you'll never misidentify your aggregates again.



Protein aggregates (left) can easily be confused with plastic ETFE (right) when you rely on morphology and intensity filters. Avoid mis-identifying aggregates with FMM, only available with Aura.

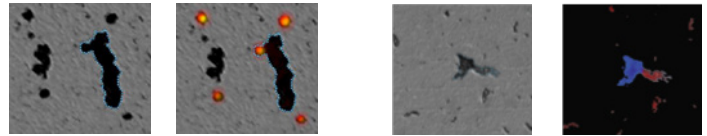


Easily identify what's cell (orange) and non-cell (black).

Easily identify what's protein (red) and non-protein (blue).


## Reliable Data at the Volume You Need

Aura delivers reproducible, quantitative data with any volume so you can use the same method throughout the development of your product. Sample limited? No problem! Aura systems does more with less so you can use 5  $\mu\text{L}$ , run triplicates and still have plenty of material left for analysis using orthogonal methods. Need to analyze 10 mL or more? Split samples into multiple wells and get summed data from [Particle Vue](#) software for your entire sample lot.

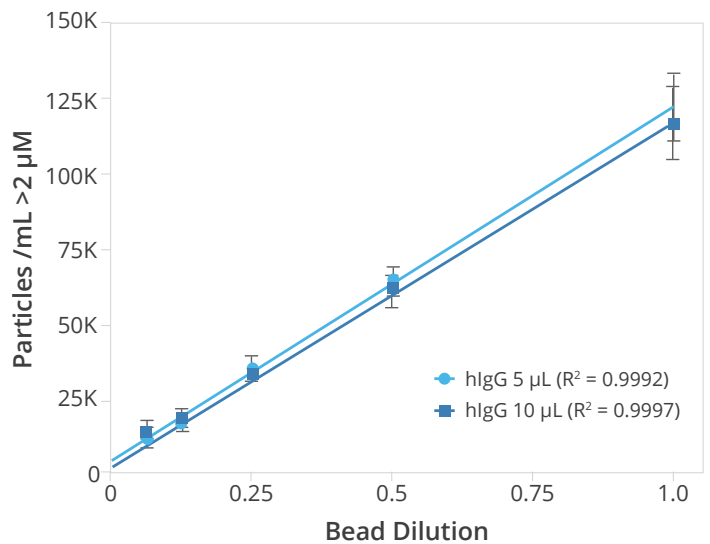

## A Closer Look with High Magnification Imaging

Got a non-biological particle in your sample and not sure what it is? Only using BMI for your particle analysis and need more information to determine what is what? Zoom in to get morphological information for Dynabeads™, fibers, and other unlabeled particles in your sample. A 20x objective on Aura+ adds another tool to your arsenal for ensuring sample purity, safety, stability, and efficacy.

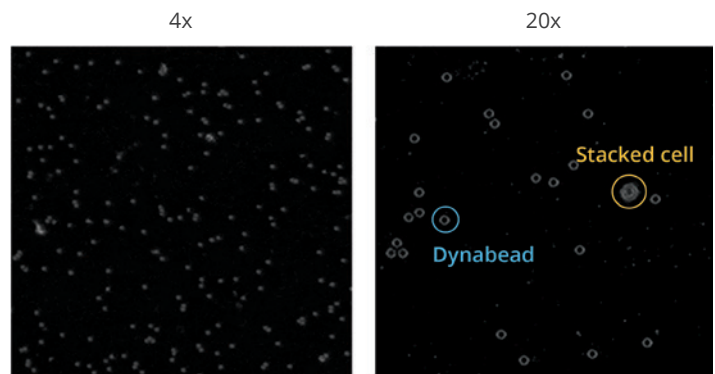

“

After evaluating all of the options for subvisible particle instruments, I concluded there really is no other choice besides getting an Aura. Nothing else can match its capabilities.

— Analytical Scientist, Major Biopharmaceutical Company





## How It Works


### BACKGROUNDED MEMBRANE IMAGING (BMI)

BMI is an analytical technique with roots in membrane microscopy, a USP 788 subvisible particle lot release method. A background image of the membrane is first taken before samples are filtered through and particles captured. The same membrane is then re-imaged – this time with particles on the surface. The background


image is subtracted so that the background texture is eliminated, revealing particles. Contrast is 10x greater than measurements performed in liquid, sizes are calibrated to an ASTM glass slide microscope, and analysis is fully automated.



Background image

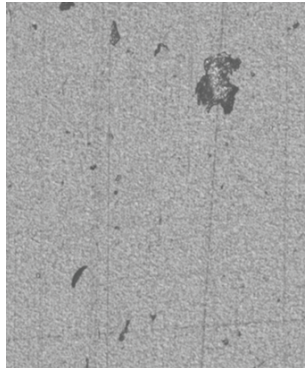

Sample image

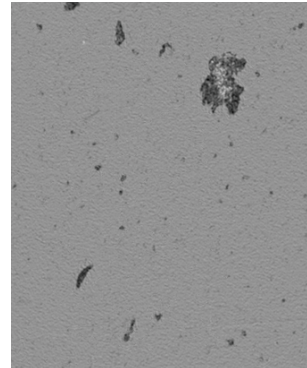


Resulting BMI image

### FLUORESCENCE MEMBRANE MICROSCOPY (FMM)

FMM works with BMI to give you a level of analysis not possible with any other particle analysis system. Targets are labeled using specific fluorescent dyes or antibodies using flexible protocols that easily fit into your workflow. Either label the particles on the membrane itself or in solution – either way it only takes a few seconds. Membranes are first

imaged with BMI to mark where particles are present. After the membrane is imaged with FMM, particles introduced from the dye itself are excluded from analysis so you don't need to worry about particles introduced from the dye.

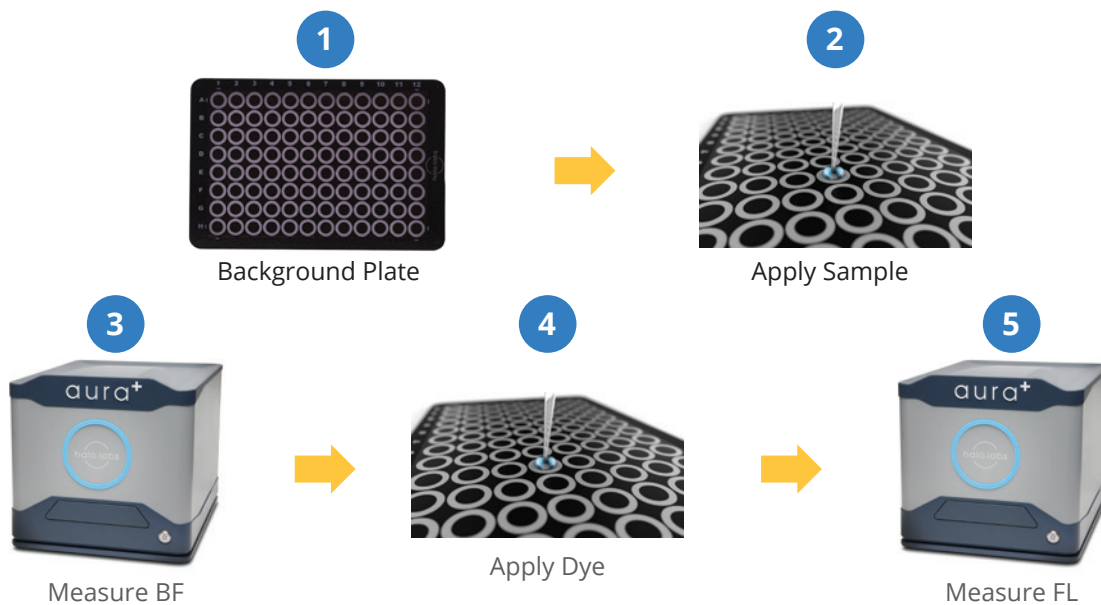

## Which Aura is Right for You?

SVP/Visible Particle Biologics Analysis	Particle Analysis & Identification	Protein Therapy/ Biologics	Gene Therapy	Cell Therapy
Aura+, Aura GT, Aura PTx, Aura CL, Aura, Aura BMI	Aura+, Aura GT, Aura PTx, Aura CL, Aura	Aura+, Aura PTx	Aura+, Aura GT,	Aura+, Aura CL

Application	Aura BMI	Aura	Aura PTx	Aura GT	Aura CL	Aura +
Particle Detection/Quantitation	✓	✓	✓	✓	✓	✓
Extrinsic Particles	✓	✓	✓	✓	✓	✓
Protein ID		✓	✓	✓	✓	✓
Polysorbate ID			✓			✓
Cell Aggregate ID					✓	✓
Capsid Aggregate ID				✓		✓
DNA Leakage				✓		✓
Immunoassays			✓	✓		✓
Cellular Assays					✓	✓
High Magnification Microscopy					✓	✓
Custom FL Applications		✓				

“

...backgrounded membrane imaging (BMI)... low volume option for particle characterization while providing significantly increased sensitivity compared to classical particle characterization methods such as light obscuration.

— Merck

## Product Specifications

<b>Imaging area</b>	24.6 mm <sup>2</sup>
<b>Brightfield illumination (BF)</b>	LED 455 nm
<b>Side Scatter illumination (SIMI)</b>	LED 465 nm
<b>Fluorescence illumination (FL)</b>	LED
<b>FL channel 1 (protein/non-protein)</b>	Ex: 440/40 nm, Em: 500/40 nm
<b>FL channel 2 options</b>	Ex: 376/30 nm, Em: 440/40 nm Ex: 482/35 nm, Em: 524/24 nm Ex: 488/50 nm, Em: 544/24 nm Ex: 540/50 nm, Em: 600/37 nm Ex: 605/50 nm, Em: 670/50 nm Custom excitation and emission
<b>Sampling efficiency</b>	100%
<b>Minimum sample volume</b>	5 µL (assay dependent)
<b>Resolution</b>	1.0 pixel/µm
<b>Particle size range (detection and quantitation)</b>	>1 µm
<b>Maximum particle concentration (1.6 µm particle size)</b>	>3,000,000 particles/mL
<b>Brightfield read time (BMI)</b>	1 minute/sample
<b>Fluorescence read time (FMM)</b>	15–30 seconds/sample
<b>Sample format</b>	96-well filter membrane
<b>Membrane type 1 (brightfield)</b>	White — polycarbonate track etched 0.4 µm or 0.8 µm pores
<b>Membrane type 2 (fluorescence)</b>	Black — polycarbonate track etched 0.4 µm pores
<b>Robotic compatibility</b>	Yes

## Instrument Product Codes

<b>Aura BMI</b>	50-1000	<b>Aura GT</b>	50-1005
<b>Aura</b>	50-1001	<b>Aura CL</b>	50-1100
<b>Aura PTx</b>	50-1006	<b>Aura+</b>	50-1101

© 2022 Halo Labs. All rights reserved. The Halo labs logo and Aura systems are trademarks and/or registered trademarks of Halo Labs. All other brands or product names mentioned are trademarks owned by their respective organizations.

Rev D